


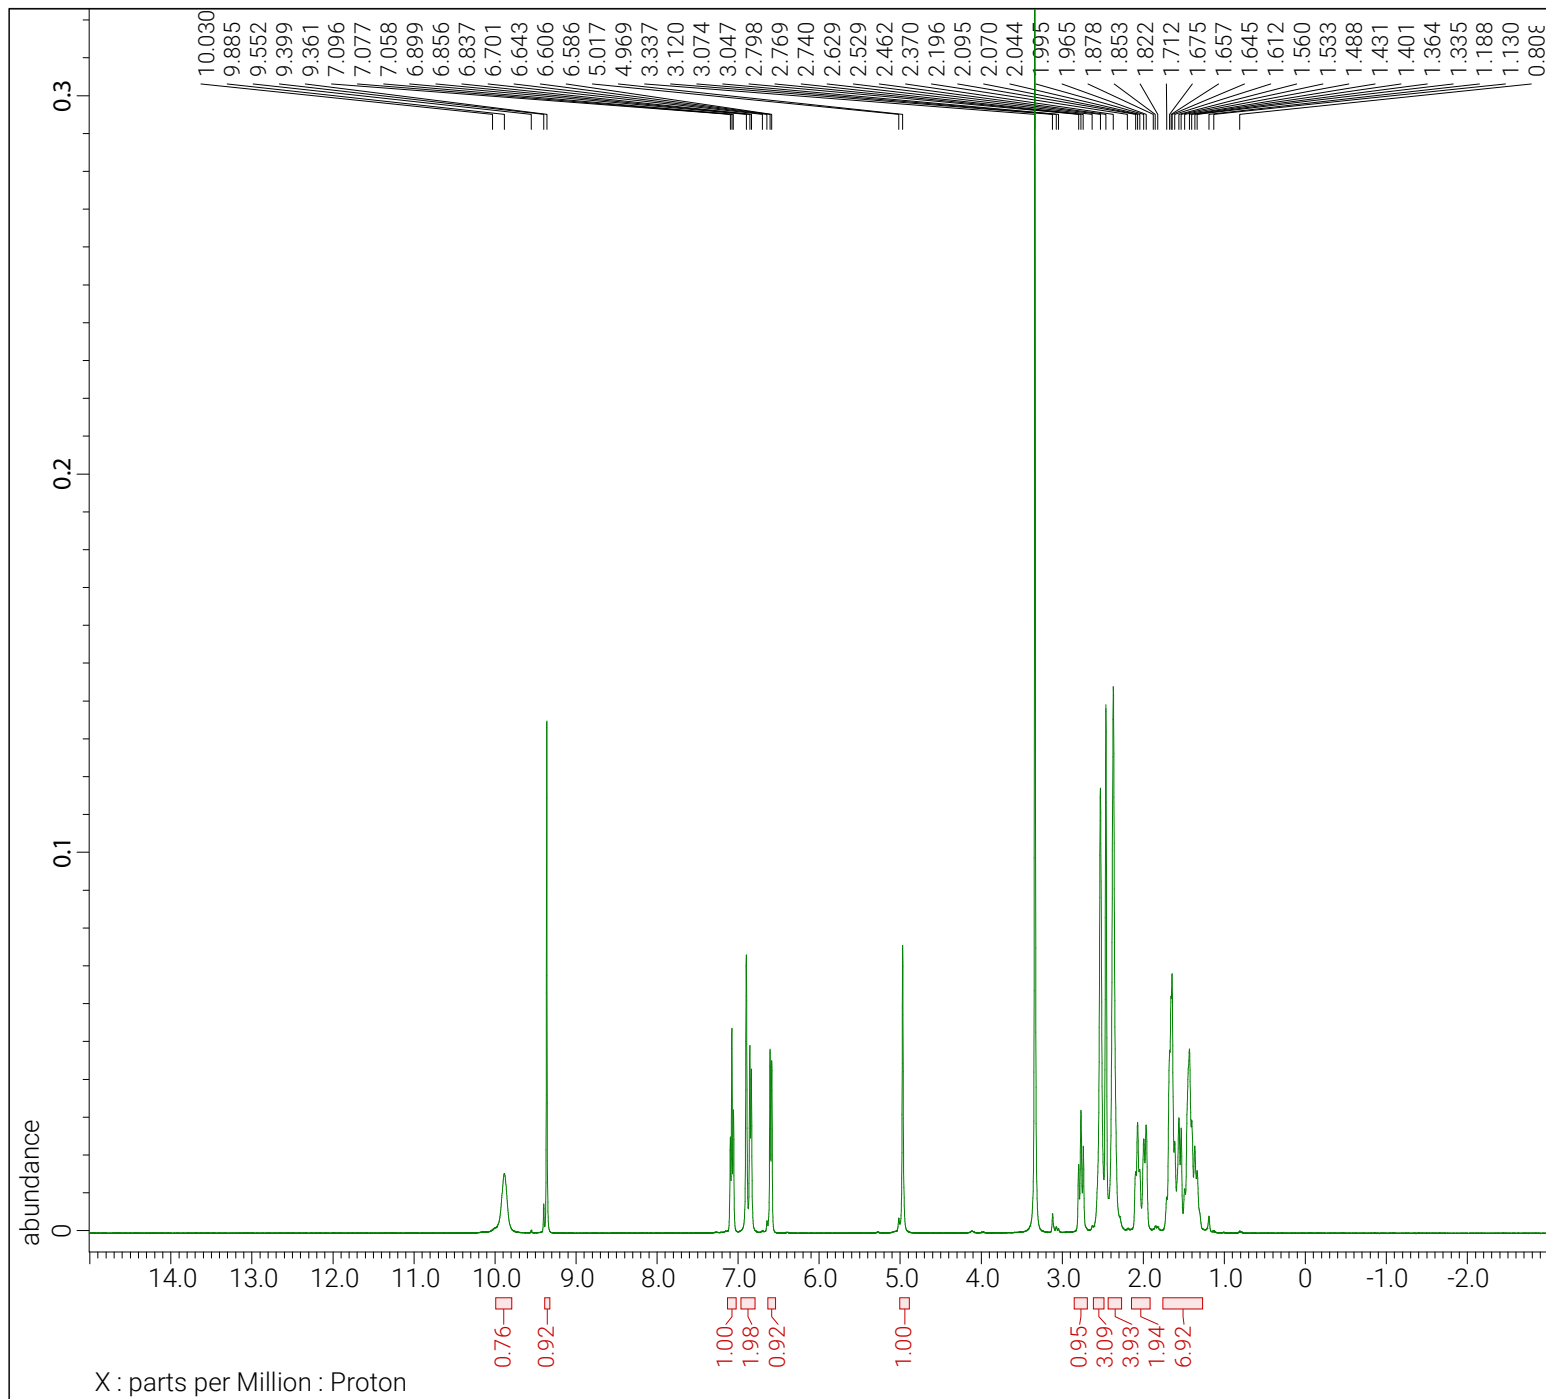

---- PROCESSING PARAMETERS ----
sexf(0.2[Hz], 0.0[s])
trapezoid(0[%], 0[%], 80[%], 100[%])
zerofill(1, TRUE)
fft(1, TRUE, TRUE)
machinephase
ppm

数据来源: 5980-20250701_proton-1-1.jdf

Filename = 5980-20250701_proton-
Author = yangyan
Experiment = proton.jxp
Sample_Id = 5980-20250701
Solvent = DMSO-D6
Actual_Start_Time = 13-AUG-2025 16:37:47
Revision_Time = 13-AUG-2025 17:44:57


Comment = single_pulse
Data_Format = 1D COMPLEX
Dim_Size = 26214
X_Domain = Proton
Dim_Title = Proton
Dim_Units = [ppm]
Dimensions = X
Spectrometer = JNM-ECZ400S/L1

Field_Strength = 9.389766[T] (400[MHz])
X_Acq_Duration = 2.2208[s]
X_Domain = Proton
X_Freq = 399.78219838[MHz]
X_Offset = 6[ppm]
X_Points = 20000
X_Prescans = 1
X_Resolution = 0.45028818[Hz]
X_Sweep = 9.00576369[kHz]
X_Sweep_Clipped = 7.20461095[kHz]
Irr_Domain = Proton
Irr_Freq = 399.78219838[MHz]
Irr_Offset = 5[ppm]
Tri_Domain = Proton
Tri_Freq = 399.78219838[MHz]
Tri_Offset = 5[ppm]
Blanking = 2.0[us]
Clipped = FALSE
Scans = 8
Total_Scans = 8

Relaxation_Delay = 3[s]
Recvr_Gain = 46
Temp_Get = 19.5[dc]
X_90_Width = 6.25[us]
X_Acq_Time = 2.2208[s]
X_Angle = 30[deg]
X_Atn = 4.5[dB]
X_Pulse = 2.08333333[us]
Irr_Mode = Off
Tri_Mode = Off

Einzelinjektionsbericht

Datei: HPLC-5980-20250701-r001.dx
Bestellname: 20250819-4
Beispielname: 5980-20250701
Instrument: QC-HPLC-019
Injektionsvolumen: 5.000
Erfassungsmethode: HPLC-1P12971-A.amx
Behandlungsmethode: HPLC-1P12971-A-20250819.pmx
Manuelle Änderung: keine
Projektname: QC-HPLC-019
Operator: Wang Xiangjun
Injektionsdatum: 2025-08-19 15:43:35+08:00
Standort: 2
Typ: Probe
Beispielinhalt: 0.00

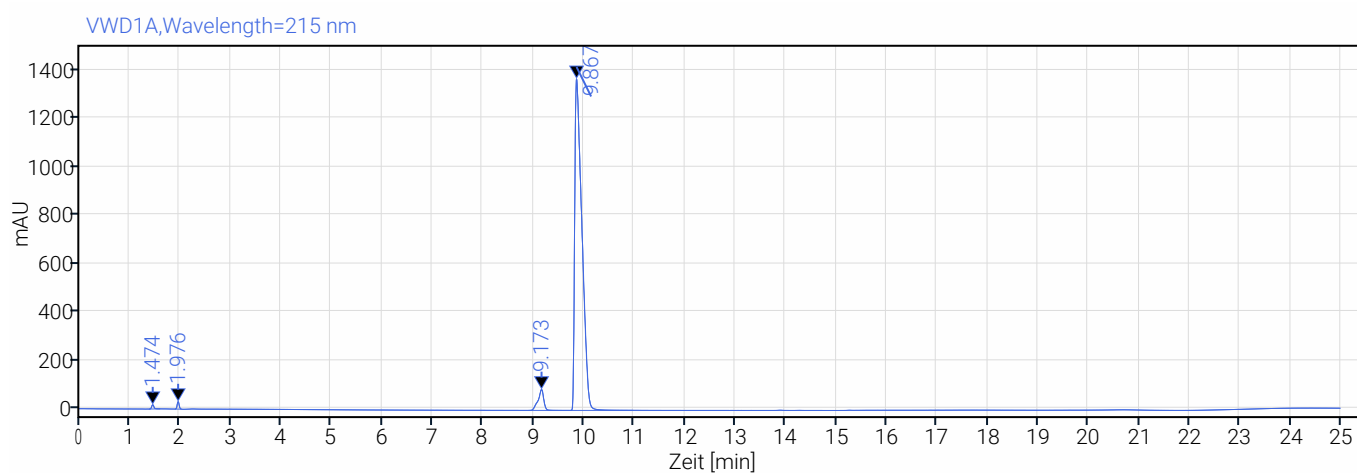

Signal: VWD1A,Wavelength=215 nm

Speicher dauer [min]	Typ	Peakband breite [min]	Gipfelfläche	hoch	Peakfläche %	Name
1.474	BBA	0.22	55.80	17.89	0.3886	
1.976	BBA	0.13	85.05	31.04	0.5923	
9.173	BB	0.81	674.38	86.63	4.6961	
9.867	BB	1.27	13545.14	1370.23	94.3231	
		Summe	14360.3700			